

Tank
Display Tank

Net size
322 liter

Reason for analysis
Routine

Barcode
XHD5-66YE-TPSL-EXEV (ID: 269420)

Created
02/29/2024

Arrived in the laboratory
03/21/2024

Evaluated
03/22/2024



Quality assessment:

The quality of your aquarium water is assessed using the score in the circle. The closer it is to 100, the better the quality. You can also use the bar chart to identify the areas in which problems may occur.

Major elements	83 / 100
Minor elements	88 / 100
Pollutants	98 / 100
Base elements	83 / 100

Results of Salt water

Base elements

Sal. total	32.66 PSU	DECREASED
Salinity	Ideal value: 35.00 PSU	Attention
KH	6.58 °dKH	DECREASED
Carbonate hardness	Ideal value: 7.50 °dKH	Attention

Major elements

Cl	18786 mg/l	TOP
Chloride	Ideal value: 18253 mg/l	Near nature
Na	9845 mg/l	TOP
Sodium	Ideal value: 10141 mg/l	Near nature
Mg	1406 mg/l	INCREASED
Magnesium	Ideal value: 1212 mg/l	Attention
S	766.1 mg/l	DECREASED
Sulfur	Ideal value: 838.9 mg/l	Attention
Ca	418.4 mg/l	TOP
Calcium	Ideal value: 388.1 mg/l	Near nature
K	402.3 mg/l	TOP
Potassium	Ideal value: 376.1 mg/l	Near nature
Br	84.66 mg/l	INCREASED
Bromine	Ideal value: 61.77 mg/l	Attention
Sr	7.87 mg/l	TOP
Strontium	Ideal value: 7.38 mg/l	Near nature
B	3.92 mg/l	TOP
Boron	Ideal value: 4.15 mg/l	Near nature
F	0.62 mg/l	TOO LITTLE
Fluorine	Ideal value: 1.20 mg/l	Critical



Minor elements

Li Lithium	241.3 µg/l Ideal value: 156.7 µg/l	TOP Near nature
Si Silicon	551.4 µg/l Ideal value: 92.19 µg/l	INCREASED Attention
I Iodine	28.06 µg/l Ideal value: 59.92 µg/l	DECREASED Attention
Ba Barium	12.75 µg/l Ideal value: 9.22 µg/l	TOP Near nature
Mo Molybdenum	2.70 µg/l Ideal value: 11.06 µg/l	TOO LITTLE Critical
Ni Nickel	0.87 µg/l Ideal value: 0.46 µg/l	TOP Near nature
Mn Manganese	--- Ideal value: 0.92 µg/l	DECREASED Attention
As Arsenic	--- Ideal value: 0.46 µg/l	TOP Near nature
Be Beryllium	--- Ideal value: 0.09 µg/l	TOP Near nature
Cr Chrome	3.82 µg/l Ideal value: 0.46 µg/l	INCREASED Attention
Co Cobalt	--- Ideal value: 0.09 µg/l	TOP Near nature
Fe Iron	13.00 µg/l Ideal value: 0.46 µg/l	TOP Near nature
Cu Copper	--- Ideal value: 0.46 µg/l	TOP Near nature
Se Selenium	--- Ideal value: 0.46 µg/l	TOP Near nature
Ag Silver	--- Ideal value: 0.09 µg/l	TOP Near nature
V Vanadium	3.50 µg/l Ideal value: 1.38 µg/l	TOP Near nature
Zn Zinc	1.64 µg/l Ideal value: 1.84 µg/l	TOP Near nature
Sn Tin	6.67 µg/l Ideal value: 0.46 µg/l	INCREASED Attention

Nutrients

NO3 Nitrate	7.10 mg/l Ideal value: 2.00 mg/l	TOP Near nature
P Phosphorus	--- Ideal value: 13.83 µg/l	TOO LITTLE Critical
PO4 Phosphate	--- Ideal value: 0.04 mg/l	TOO LITTLE Critical

Pollutants

Al.	70.45 µg/l	INCREASED
Aluminium	Ideal value: 0.09 µg/l	Attention
Sb	---	TOP
Antimony	Ideal value: 0.09 µg/l	Near nature
Bi	---	TOP
Bismuth	Ideal value: 0.09 µg/l	Near nature
Pb	---	TOP
Lead	Ideal value: 0.09 µg/l	Near nature
Cd	---	TOP
Cadmium	Ideal value: 0.18 µg/l	Near nature
La.	---	TOP
Lanthanum	Ideal value: 0.00 µg/l	Near nature
Tl	---	TOP
Thallium	Ideal value: 0.09 µg/l	Near nature
Ti	---	TOP
Titanium	Ideal value: 0.09 µg/l	Near nature
W	---	TOP
Tungsten	Ideal value: 0.00 µg/l	Near nature
Hg	---	TOP
Mercury	Ideal value: 0.00 µg/l	Near nature

Results of Osmosis water

Minor elements

Li	---	TOP
Lithium	Ideal value: 0.00 µg/l	Near nature
Si	---	TOP
Silicon	Ideal value: 0.00 µg/l	Near nature
Ba	---	TOP
Barium	Ideal value: 0.00 µg/l	Near nature
Mo	---	TOP
Molybdenum	Ideal value: 0.00 µg/l	Near nature
Ni	---	TOP
Nickel	Ideal value: 0.00 µg/l	Near nature
Mn	---	TOP
Manganese	Ideal value: 0.00 µg/l	Near nature
As	---	TOP
Arsenic	Ideal value: 0.00 µg/l	Near nature
Be	---	TOP
Beryllium	Ideal value: 0.00 µg/l	Near nature
Cr	---	TOP
Chrome	Ideal value: 0.00 µg/l	Near nature
Co	---	TOP
Cobalt	Ideal value: 0.00 µg/l	Near nature
Fe	---	TOP
Iron	Ideal value: 0.00 µg/l	Near nature
Cu	---	TOP
Copper	Ideal value: 0.00 µg/l	Near nature
Se	---	TOP
Selenium	Ideal value: 0.00 µg/l	Near nature
Ag	---	TOP
Silver	Ideal value: 0.00 µg/l	Near nature
V	---	TOP
Vanadium	Ideal value: 0.00 µg/l	Near nature
Zn	---	TOP
Zinc	Ideal value: 0.00 µg/l	Near nature
Sn	---	TOP
Tin	Ideal value: 0.00 µg/l	Near nature

Nutrients

P	---	TOP
Phosphorus	Ideal value: 0.00 µg/l	Near nature
PO4	---	TOP
Phosphate	Ideal value: 0.00 mg/l	Near nature

Pollutants

Al. Aluminium	---	TOP Near nature
Sb Antimony	---	TOP Near nature
Bi Bismuth	---	TOP Near nature
Pb Lead	---	TOP Near nature
Cd Cadmium	---	TOP Near nature
La. Lanthanum	---	TOP Near nature
Tl Thallium	---	TOP Near nature
Ti Titanium	---	TOP Near nature
W Tungsten	---	TOP Near nature
Hg Mercury	---	TOP Near nature

Recommendations

The following recommendations were calculated for the aquarium **Display Tank** with **322 liters** content.

Recommended actions

Phosphorus Dose 3.22 ml Nutrition P per day. Reduce the dose if the home test shows more than 0.03 mg/l PO ₄ .	Important
Magnesium Stop adding magnesium to reduce value to 1300-1350 mg/l.	Recommended
Bromine Reduce/stop addition of bromide to bring value down to 65-67 mg/l.	Recommended
Silicon Silicon is elevated. Find the cause and eliminate it (e.g. RO water, frozen food,...).	Recommended
Carbonate hardness Increase the KH value to 7 to 8 °dKH. For this purpose, dose e.g. once 29.62 ml Essentials+ #1 or 20.74 ml Essentials pro #1 into your aquarium.	Recommended
Salinity Increase the salinity to 35 PSU. For example, add 1287 ml Absolute Ocean #1 and 1287 ml Absolute Ocean #2 to the aquarium.	Recommended

Iodine (I -1000 ml bottle)

Important

Addition Total: 10.26 ml
Divide the addition into portions: twice 5.13 ml *

Iodine (I -alt. 100 ml bottle)

Important

Addition Total: 1.03 ml
Divide the addition into portions: twice 0.51 ml *

Molybdenum (Mo)

Recommended

Addition Total: 13.46 ml
Divide the addition into portions: twice 6.73 ml *

Manganese (Mn)

Recommended

Addition Total: 1.48 ml
Divide the addition into portions: once 1.48 ml


Fluorine (F)

Recommended

Addition Total: 93.61 ml
Divide the addition into portions: three times 31.2 ml *

* Only one portion should be dosed per day.

Diagrams

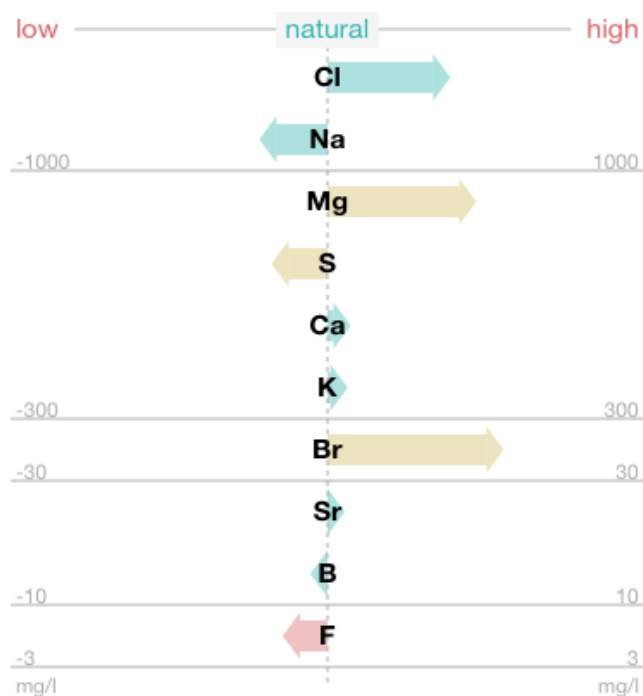

Composition of the aquarium water


The diagram shows whether the concentrations of the major elements in your water sample match the measured salinity or whether individual elements are increased or reduced. Note the different concentration ranges on the x-axis.

Background: Natural seawater consists of the same elements in fixed proportions. Only the concentrations of the elements increase or decrease in proportion to salinity. That is why the ideal values also change with salinity.

Green arrow
Value is relatively natural.

Yellow arrow
Value is becoming increasingly unnatural.

Red arrow
Value unnatural.

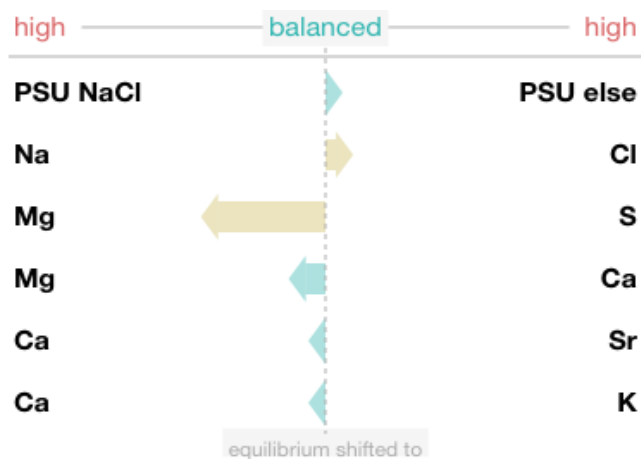

Element ratios

This chart shows whether the element supply is appropriate or whether the ratios of certain element pairs are skewed due to an imbalanced supply. The arrow points in the direction of the element with increased concentration. Only the relationship between the elements is evaluated. The evaluation of the individual measured values may vary.

Background: The reef inhabitants remove various elements from the aquarium water. To compensate for this consumption and obtain water that is true to nature, water changes are carried out and water additives are used. This does not always work as needed.

Green Arrow


Relationship close to nature.

Yellow arrow

Ratio slightly shifted.

Red arrow

Ratio shifted drastically.

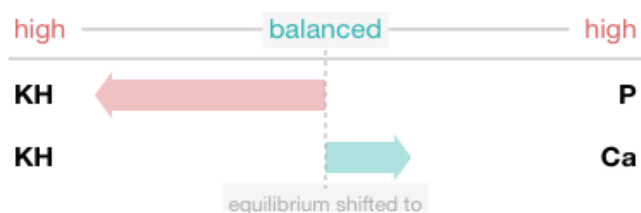

Growth Factors

This diagram shows whether important growth factors are in balance or out of proportion. The arrow points in the direction of the factor with increased concentration. Only the relationship between the factors is evaluated. The evaluation of the individual measured values may vary.

Background: The most important growth factors include carbonate hardness, calcium concentration and phosphorus content. When these values are slightly increased, growth is usually encouraged, while greatly increased or reduced values slow growth. If there is an imbalance between these factors, it can adversely affect coral growth and, in the worst case, lead to tissue necrosis.

Green arrow

Balance between factors OK.

Yellow arrow

Factors increasingly disproportionate to one another.

Red arrow

Factors in disproportion to one another.